


Vision Screening Certificate

Vision Screening must be conducted regularly as eyes may change over time.

Vision Screening doesn't replace a complete eye examination by an ophthalmologist or optometrist.

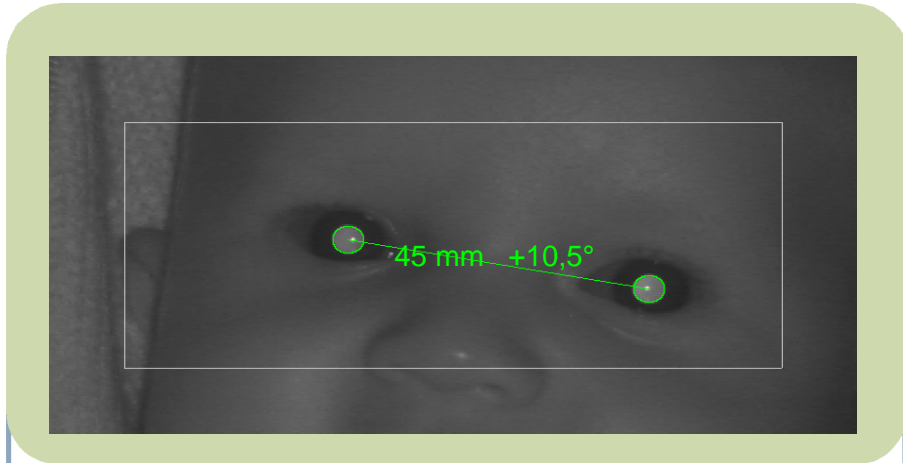

02/02/2006
Date of measurement

Name

Müller

Surname

Lieschen

Date of birth


01/21/2005



Screening performed at:

Dr. Mustermann
Praxissgasse 22
90411 Arzthausen
Tel.: 0234/12345678
Fax.: 0234/12345679

by: Verona

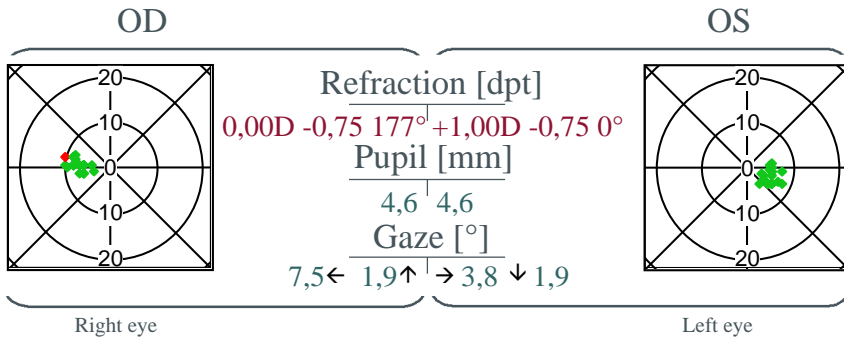

Pass/Refer Criteria

All measurements were completed successfully.

The difference between the sphere value of each eye is less than 1.0 dpt.
The difference between the cylinder value of each eye is less than 1.0 dpt.

The cylinder value of each eye is less than 1.0 dpt.

The sphere value of each eye is between -1.0 and +1.0 dpt.

The difference between the pupil diameter of each eye is less than 1.0 mm.

Yes

No

Vision Screening powered by
www.plusoptix.de

plusoptix
eye·vision·technology

Refer